



Keywords: high-speed ADCs, analog to digital converters, coherent sampling, input test tone, sinewave testing, clock frequency, sampling frequency, equipment, low phase noise, signal generator, logic analyzer, synthesizer, data acquisition software, MATLAB Dec 18, 2002

APPLICATION NOTE 1819

Selecting the Optimum Test Tones and Test Equipment for Successful High-Speed ADC Sinewave Testing

Abstract: An earlier application note, "Coherent Sampling vs. Window Sampling," covered the basics of coherent sampling. It showed differences between tests performed with coherent sampling and windowed sampling conditions. The following technical discussion is a follow-up note, which deals with the proper selection of test tones and instruments to successfully test and evaluate a high-speed ADC's AC performance.

Also see:

- Application note 3190, "[Coherent Sampling Calculator \(CSC\)](#)"
- [Coherent Sampling Calculator](#) (XLS, 81K)

As discussed in the earlier application note 1040, "[Coherent Sampling vs. Window Sampling](#)," a variety of approaches may be used to evaluate dynamic performance parameters, such as signal-to-noise ratio (SNR), signal-to-noise and distortion (SINAD), total harmonic distortion (THD), intermodulation distortion (IMD) and spurious-free dynamic range (SFDR) of high speed data converters. However, the concept of coherent sampling, a frequency-based sinewave test, yields more accurate and repeatable test results than using a windowing method.

In sinewave-testing a high-speed analog-to-digital converter (ADC), it is not only imperative to sample the applied waveform continuously to avoid unwanted artifacts in the FFT spectrum, but to precisely select the sampling frequency (f_{SAMPLE}), the input test tone (f_{IN}), and the size of the data record (N_{RECORD}). For any given clock frequency there exist certain input test tones, which can hide ADC errors, while other frequencies reveal ADC errors. These frequencies can vary by only a fraction of a percent and yield vastly different results. The optimum input test tone is one for which there are N_{RECORD} distinct phases sampled, which are uniformly distributed between 0 and 2π radians. Taking this knowledge into account, coherent sampling can be described as the sampling of a periodic signal, where an integer number of its cycles fit into a predefined sampling window. Mathematically, this is expressed by

$$f_{\text{IN}} = (N_{\text{WINDOW}}/N_{\text{RECORD}}) \times f_{\text{SAMPLE}}$$

where f_{IN} is a continuous sinusoidal input signal, f_{SAMPLE} is the ADC's clock/sample frequency, N_{WINDOW} represents an integer number of cycles within the sampling window, and N_{RECORD} is the number of data points targeted for the sampling window or FFT.

Additionally it is important to choose N_{RECORD} large enough to produce at least one representative sample of every frequency bin² of the converter. Given that the input tone is chosen as previously discussed, an ideal converter's transfer curve (excluding random noise) requires the minimum value for N_{RECORD} to be $\pi^2 N$, where N is the resolution of the data converter under test.

There are two common ways to calculate the desired input tone. Following are examples of these two methods

based on coherent sampling. Assuming that an ADC, such as the MAX1190, is driven with a 120MHz clock, and a near optimum input frequency of 17MHz is to be analyzed with an 8192-point FFT record, the following two steps provide guidance in selecting the appropriate input test tone.

1. Start with $f_{IN} = 17\text{MHz}$ and $f_{SAMPLE} = 120\text{MHz}$ to determine the window size N_{WINDOW} (remember that according to the previous discussion, N_{WINDOW} has to be an integer odd or mutually prime number) for an 8192-point data record N_{RECORD} .

$$N_{WINDOW} = \text{int} (f_{IN}/f_{SAMPLE}) \times N_{RECORD}$$
$$N_{WINDOW} = \text{int} (17\text{MHz}/120\text{MHz}) \times 8192 = 1160$$

2. Based on the above result for N_{WINDOW} , the next closest mutually prime (odd) number is 1163 (1161). Use either of these numbers to compute the final, near-optimum input test tone as follows

$$f_{IN} = f_{SAMPLE} \times (N_{WINDOW}/N_{RECORD})$$
$$f_{IN}(\text{MUTUALLY_PRIME}) = 120\text{MHz} \times (1163/8192) = 17.0361328\text{MHz}$$
$$f_{IN}(\text{ODD}) = 120\text{MHz} \times (1161/8192) = 17.0068359\text{MHz}$$

Unfortunately, this very method will require a high-resolution signal synthesizer capable of supporting all the digits necessary to get an accurate reading on the input frequency. A different approach, which offsets the clock frequency from its exact value of 120MHz, yet still, obeying the rules for coherent sampling, can overcome such stringent demand. The next five steps show that the need for a high-resolution instrument is relaxed by 'distributing' the number of required digits between input and sampling frequency.

1. Determine the resolution of the sampling frequency that fits into an 8192-point record by

$$\Delta f = f_{SAMPLE}/N_{RECORD}$$
$$\Delta f = 120\text{MHz}/8192 = 14.6484375\text{kHz}$$

2. Some of commonly available signal generators in the market may not offer enough resolution to offer this many digits to accurately capture both input and sampling frequency. To bypass this requirement and still meet the coherent sampling condition, it is recommended to select Δf based on the next highest integer number.

$$\Delta f = \text{int} (f_{SAMPLE}/N_{RECORD}) = 15\text{kHz}$$

3. Based on the new Δf , the exact sampling frequency computes to

$$f_{SAMPLE} = \Delta f \times N_{RECORD}$$
$$f_{SAMPLE} = 15\text{kHz} \times 8192 = 122.880\text{MHz}$$

4. Δf also helps to determine the size of N_{WINDOW} . Again, use the next highest integer odd (or mutually prime) number, determined by the desired input test tone and Δf .

$$N_{WINDOW} = \text{int} (f_{IN}/\Delta f)$$
$$N_{WINDOW} = 17\text{MHz}/15\text{kHz} = 1133$$

5. Based on these findings, the near optimum input test tone f_{IN} calculates as follows

$$f_{IN} = f_{SAMPLE} \times (N_{WINDOW}/N_{RECORD})$$
$$f_{IN} = 122.88\text{MHz} (1133/8192) = 16.995\text{MHz}$$

Equipment and Set-Up Recommendations for a Successful High-Speed ADC Test

Table 1 lists some recommended hardware instruments and software products, which have proven to be quite valuable for data capture and analysis of high-speed ADC dynamic performance parameters.

Table 1. Equipment and software tool recommendations for high-speed ADC testing.

Type Of Equipment	Equipment Count and Notes
Synthesized Signal Generator: HP/Agilent 8662/3A (10kHz to 1.28/2.56GHz, -139dBm to +13dBm) or HP/Agilent 8644A (252kHz to 1.030GHz, -140dBm to +20dBm)	2 generators for single-channel ADC input and clock 3 generators for IMD test (single-channel ADC) or 3 generators for dual-channel ADC inputs and clock 4 generators for IMD test (dual-channel ADC)
Logic Analyzer System: HP/Agilent 16500C mainframe (or similar) (1Gsps State Analyzer Card HP16517A optional and for ADCs with sampling speeds >100MHz only)	1 Logic analyzer (in default configuration, allows to evaluate up to 4 channels for ADCs with up to 16-bit resolution)
Band-Pass Filters: TTE's Q56/KC7 series for frequencies <100MHz/>100MHz (Other suitable filter suppliers are Allen Avionics or K&L Microwave)	1 Filter for single-channel ADC 2 Filters for simultaneous evaluation of a dual- channel ADC
Power Combiner: Mini-Circuits 15542 ZSC-2-1W (or similar)	1 Combiner (used for two-tone IMD evaluation only)
RF Frequency Balun/Transformer: MA/COM H-9-SMA (or similar)	2 Baluns for single-channel ADC and clock 3 Baluns for dual-channel ADC and clock
GPIO-Compatible Interface Card: National Instruments GPIB/IEEE®-488 Interface Card + driver and installation software (PC-/PCMCIA-card or GPIB-to-USB port adapter)	1 Interface card Note: This card is recommended for fast data transfer between logic analyzer and computer; requires C-based software platform (e.g. LabWindows/CVI) to control the interface. Data can also be extracted from the logic analyzer with a floppy disk.
Data Analysis Software: MATLAB from The Math Works Inc. or Measurement Studio with LabWindows/CVI from National Instruments	1 License for each software package Note: LabWindows/CVI provides a C-based platform to control the interface between logic analyzer and PC

Probably the most critical elements in such a test setup (**Figure 1**) are the synthesized signal generators, used to generate the waveforms for the clock and input frequencies. Suitable signal generators must feature low phase noise; because measured dynamic parameters such as SNR will degrade dramatically with an increase in phase noise "[Defining and Testing Dynamic Parameters in High-Speed ADCs, Part 1.](#)" Furthermore, these signal synthesizers have to provide adequate output power, must have phase locking capabilities, and a frequency resolution of 0.1Hz or better to ensure accurate coherence.

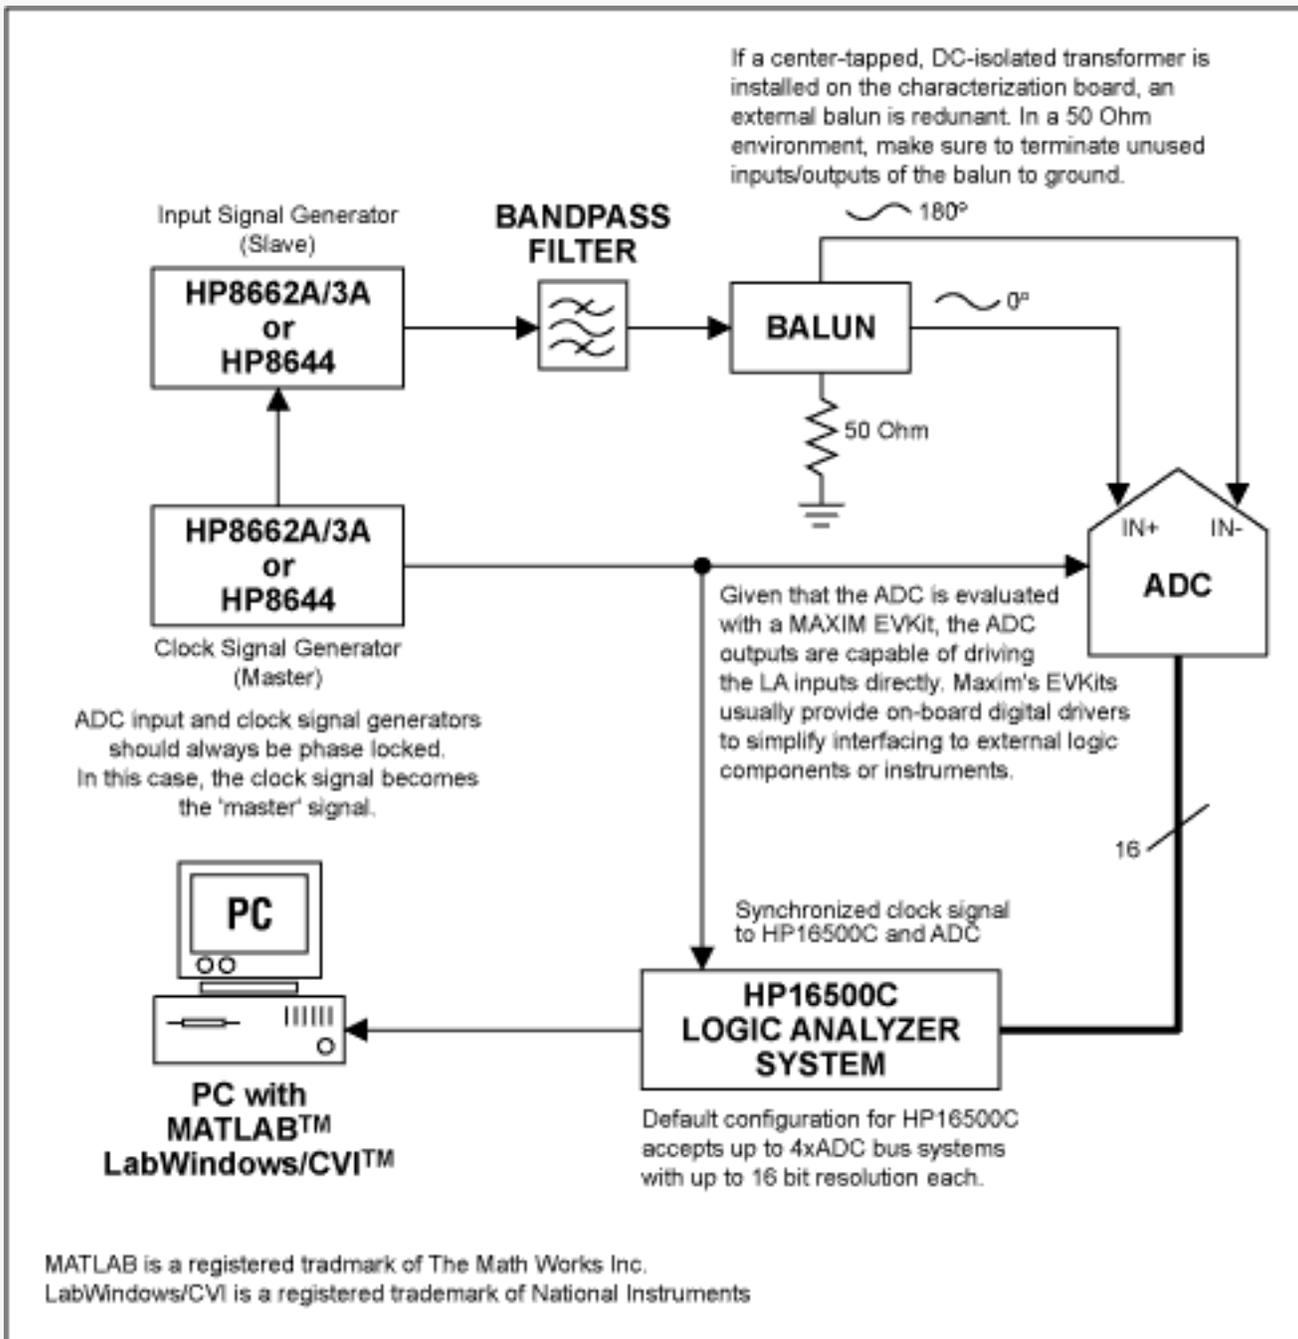


Figure 1.

Although generators such as the HP8662A series from Hewlett-Packard/Agilent are rather expensive and have a limited output amplitude range of -139dBm to +13dBm (0.025 μ V_{RMS} to 1V_{RMS} into a 50 Ω load), they satisfy all other test requirements and are most suitable for the dynamic tests of high-speed converters.

To further reduce the harmonic distortion components of the synthesizer's output frequency it is recommended to filter the desired test tone by applying a high-quality bandpass between generator and ADC input drive.

Clock and signal inputs of fast ADCs usually are equipped with true differential input architectures, which require the signal generator's single-ended output to be converted to a differential signal. This can be achieved by using an external balun or an off-the-shelf transformer with center tap and DC isolation. Usually, the latter is a surface-mount component and should be incorporated on the characterization board, used to test the ADC. Most of Maxim's high-speed data converter evaluation kits feature such transformers and emphasize on impedance matched I/O lines to keep unwanted signal skew and phase mismatch at a minimum.

To capture digital data on the parallel output ports of a high-speed ADC a fast Logic Analyzer will be needed. An excellent choice is the Hewlett-Packard/Agilent HP16500 Logic Analyzer mainframe. For converter sampling/clock speeds greater than 100MHz, this system accepts high-speed data capture cards such as the HP16517A. The

system's mainframe features a GPIB/HPIB bus, capable of interfacing with a PC-based GPIB to transmit data from the Logic Analyzer to a PC quickly. One may of course use the floppy drive built into the instrument to store data, however depending on the size of the data record (number of points in the FFT) this may take significantly longer than just utilizing the analyzer's GPIB interface. Once data has been sent to the PC, a signal processing software such as MATLAB may be used to analyze the data records from the logic analyzer. The following MATLAB sample code maybe used to calculate the basic AC specifications of any a high-speed ADC.

%Source Code Sample MAX144X Family

%The following program code plots the FFT spectrum of a desired test tone. Test tone based on coherent sampling criteria, and

%computes SNR, SINAD, THD and SFDR.

%Copyright Au/Hofner, Maxim Integrated Products, 120 San Gabriel Drive, Sunnyvale, CA94086

%This program is believed to be accurate and reliable. This program may get altered without prior notification.;

```
disp('HP16500C LA 100/110 State Card');
filename=input('Enter file name or press RETURN to accept data from LA via GPIB/HPIB): ');
if isempty(filename)
    filename = 'listing';
end
fid=fopen(filename,'r');
numpt=input('Number of Points in FFT? ');
fclk=input('Sampling Frequency (MHz)? ');
numbit=input('ADC Resolution? ');

%Discard first 13 lines of the LA listing (LA header), as they don't contain valid data.
for i=1:13,
    fgetl(fid);
end
[v1,count]=fscanf(fid,'%f',[2,numpt]);
fclose(fid);
v1=v1';
code=v1(:,2);

%Warning: ADC output may be clipping - reduce input amplitude
if (max(code)==2numbit-1) | (min(code)==0)
    disp('WARNING: ADC OUTPUT MAYBE CLIPPING - CHECK INPUT AMPLITUDE!');
end

figure;
plot([1:numpt],code);
title('TIME DOMAIN')
xlabel('SAMPLES');
```

```

ylabel('DIGITAL OUTPUT CODE');
Dout=code-(2^numbit-1)/2;      %Re-center the digitized sinusoidal input
Doutw=Dout;
Dout_spect=fft(Doutw);
Dout_dB=20*log10(abs(Dout_spect));
figure;
maxdB=max(Dout_dB(1:numpt/2));
plot([0:numpt/2-1].*fclk/numpt,Dout_dB(1:numpt/2)-maxdB);
grid on;
title('FFT PLOT');
xlabel('ANALOG INPUT FREQUENCY (MHz)');
ylabel('AMPLITUDE (dB)');
a1=axis; axis([a1(1) a1(2) -100 a1(4)]);
fin=find(Dout_dB(1:numpt/2)==maxdB); %Find the signal bin (DC represents bin=1)
span=max(round(numpt/200),5); %Determine span of input frequency on each side
spanh=2; %Search span for harmonic distortion components on each side
spectP=(abs(Dout_spect)).*(abs(Dout_spect)); %Determine power level
Pdc=sum(spectP(1:span)); %Determine DC offset power level
Ps=sum(spectP(fin-span:fin+span)); %Determine signal power level
Fh=[]; %Vector storing frequency and power components of signal and harmonics
Ph=[]; %HD1=signal, HD2=2nd harmonic, HD3=3rd harmonic, etc.

%Find the harmonic frequencies/power within the FFT plot
for har_num=1:10
    tone=rem((har_num*(fin-1)+1)/numpt,1); %Note: tones > fSAMPLE are aliased back
    if tone>0.5
        tone=1-tone;
    end
    Fh=[Fh tone];
end

%For this method to work properly, make sure that the folded back high order harmonics do not overlap with DC and signal
%components or lower order harmonics.
har_peak=max(spectP(round(tone*numpt)-spanh:round(tone*numpt)+spanh));
har_bin=find(spectP(round(tone*numpt)-spanh:round(tone*numpt)+spanh)==har_peak);
har_bin=har_bin+round(tone*numpt)-spanh-1; Ph=[Ph sum(spectP(har_bin-1:har_bin+1))];

```

```

end

Pd=sum(Ph(2:5));           %Total distortion power level
Pn=sum(spectP(1:
numpt/2))-Pdc-Ps-Pd;      %Extract noise power level
format;
A=(max(code)-min
(code))/2^numbit          %Analog input amplitude in mV
AdB=20*log10(A)           %Analog input amplitude in dB
SNR=10*log10(Ps/Pn)       %SNR in dB
SNR=10*log10(Ps/Pn)       %SINAD in dB
SINAD=10*log10(Ps/(Pn+Pd))
disp('THD - HD2 through HD5');
THD=10*log10(Pd/Ph(1))    %THD in dB
SFDR=10*log10(Ph(1)/
max(Ph(2:10)))           %SFDR in dB
disp('SIGNAL AND HARMONIC POWER (dB)');
HD=10*log10(Ph(1:10)/Ph(1))

hold on;
plot(Fh(2)*fclk,0,'mo',Fh(3)*fclk,0,'cx',Fh(4)*fclk,0,'r+',Fh(5)*fclk,0,'gx',Fh(6)*fclk,0,'bs',Fh(7)*fclk,0,'bd',
Fh(8)*fclk,0,'kv',
Fh(9)*fclk,0,'y^');
legend('SIGNAL','HD2','HD3','HD4','HD5','HD6','HD7','HD8','HD9');
hold off;

```

Conclusion

This application note provides one approach to establishing dynamic performance parameters of a high-speed ADC quickly and precisely. Digital data can also be analyzed using a high dynamic performance, high-resolution DAC in combination with an output filter and spectrum analyzer. However, that approach requires careful selection and design of the reconstruction signal path to avoid falsifying the ADCs true dynamic performance. Some applications may even prefer a test system with built-in digital distortion analyzer. Even a Logic Analyzer can deliver a quick, but rather inaccurate analysis of the digital output signals. Just remember: Choosing the appropriate configuration for your test setup entirely depends on the type of application, available hardware and software resources, design time, and the quality of dynamic performance results needed for your application.

References

1. Application note 1040, "[Coherent Sampling vs. Window Sampling](#)"
2. Application note 728, "[Defining and Testing Dynamic Parameters in High-Speed ADCs, Part 1](#)"
3. Application note 729, "[Dynamic Testing of High-Speed ADCs, Part 2](#)"

Notes

1. If N_{RECORD} is a power-of-two value, then an odd number for N_{WINDOW} will meet the coherent sampling requirement.
2. The size of an ideal frequency bin is defined by $\text{bin} = f_{\text{SAMPLE}}/N_{\text{RECORD}}$.

Related Parts

MAX1180: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1181: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1182: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1183: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1184: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1185: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1186: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1190: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1191: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1192: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1193: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1195: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1196: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1197: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1198: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1206: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1207: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1208: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1209: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1211: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1444: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1446: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1448: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)
MAX1449: [QuickView](#) -- [Full \(PDF\) Data Sheet](#) -- [Free Samples](#)

Automatic Updates

Would you like to be automatically notified when new application notes are published in your areas of interest? [Sign up for EE-Mail™](#).

Application note 1819: www.maxim-ic.com/an1819

More Information

For technical support: www.maxim-ic.com/support

For samples: www.maxim-ic.com/samples

Other questions and comments: www.maxim-ic.com/contact

AN1819, AN 1819, APP1819, Appnote1819, Appnote 1819

Copyright © by Maxim Integrated Products

Additional legal notices: www.maxim-ic.com/legal